

Batch ID/RT Job Number
 Batch Residence Time
 CHL+
 Pre Reaction PCB / Moisture (ppm)
 Reagent Amount / Catalyst H2O
 Batch Reaction Time (Min)
 Post Reaction PCB (ppm)
 Batch Amount (Gallons)
 Batch Residence Time Stop
 Gallons Out / Destination Tank
 Mixing Tank

are

number

Number

Reaction:

Reabsorption (liters)

Batch:

Bag
Pod

[illegible]

MT-3

Fil Tr2 KANS

1

100

1

Age Group	Percentage of Respondents
18-29	85%
30-49	80%
50-69	75%
70+	70%

2007-2008-2009-2010-2011-2012-2013-2014-2015-2016-2017-2018-2019-2020-2021-2022-2023-2024-2025-2026-2027-2028-2029-2030-2031-2032-2033-2034-2035-2036-2037-2038-2039-2040-2041-2042-2043-2044-2045-2046-2047-2048-2049-2050-2051-2052-2053-2054-2055-2056-2057-2058-2059-2060-2061-2062-2063-2064-2065-2066-2067-2068-2069-2070-2071-2072-2073-2074-2075-2076-2077-2078-2079-2080-2081-2082-2083-2084-2085-2086-2087-2088-2089-2090-2091-2092-2093-2094-2095-2096-2097-2098-2099-2100-2101-2102-2103-2104-2105-2106-2107-2108-2109-2110-2111-2112-2113-2114-2115-2116-2117-2118-2119-2120-2121-2122-2123-2124-2125-2126-2127-2128-2129-2130-2131-2132-2133-2134-2135-2136-2137-2138-2139-2140-2141-2142-2143-2144-2145-2146-2147-2148-2149-2150-2151-2152-2153-2154-2155-2156-2157-2158-2159-2160-2161-2162-2163-2164-2165-2166-2167-2168-2169-2170-2171-2172-2173-2174-2175-2176-2177-2178-2179-2180-2181-2182-2183-2184-2185-2186-2187-2188-2189-2190-2191-2192-2193-2194-2195-2196-2197-2198-2199-2200-2201-2202-2203-2204-2205-2206-2207-2208-2209-2210-2211-2212-2213-2214-2215-2216-2217-2218-2219-2220-2221-2222-2223-2224-2225-2226-2227-2228-2229-2230-2231-2232-2233-2234-2235-2236-2237-2238-2239-2240-2241-2242-2243-2244-2245-2246-2247-2248-2249-2250-2251-2252-2253-2254-2255-2256-2257-2258-2259-2260-2261-2262-2263-2264-2265-2266-2267-2268-2269-2270-2271-2272-2273-2274-2275-2276-2277-2278-2279-2280-2281-2282-2283-2284-2285-2286-2287-2288-2289-2290-2291-2292-2293-2294-2295-2296-2297-2298-2299-2300-2301-2302-2303-2304-2305-2306-2307-2308-2309-2310-2311-2312-2313-2314-2315-2316-2317-2318-2319-2320-2321-2322-2323-2324-2325-2326-2327-2328-2329-2330-2331-2332-2333-2334-2335-2336-2337-2338-2339-2340-2341-2342-2343-2344-2345-2346-2347-2348-2349-2350-2351-2352-2353-2354-2355-2356-2357-2358-2359-2360-2361-2362-2363-2364-2365-2366-2367-2368-2369-2370-2371-2372-2373-2374-2375-2376-2377-2378-2379-2380-2381-2382-2383-2384-2385-2386-2387-2388-2389-2390-2391-2392-2393-2394-2395-2396-2397-2398-2399-2400-2401-2402-2403-2404-2405-2406-2407-2408-2409-2410-2411-2412-2413-2414-2415-2416-2417-2418-2419-2420-2421-2422-2423-2424-2425-2426-2427-2428-2429-2430-2431-2432-2433-2434-2435-2436-2437-2438-2439-2440-2441-2442-2443-2444-2445-2446-2447-2448-2449-2450-2451-2452-2453-2454-2455-2456-2457-2458-2459-2460-2461-2462-2463-2464-2465-2466-2467-2468-2469-2470-2471-2472-2473-2474-2475-2476-2477-2478-2479-2480-2481-2482-2483-2484-2485-2486-2487-2488-2489-2490-2491-2492-2493-2494-2495-2496-2497-2498-2499-2500-2501-2502-2503-2504-2505-2506-2507-2508-2509-2510-2511-2512-2513-2514-2515-2516-2517-2518-2519-2520-2521-2522-2523-2524-2525-2526-2527-2528-2529-2530-2531-2532-2533-2534-2535-2536-2537-2538-2539-2540-2541-2542-2543-2544-2545-2546-2547-2548-2549-2550-2551-2552-2553-2554-2555-2556-2557-2558-2559-2560-2561-2562-2563-2564-2565-2566-2567-2568-2569-2570-2571-2572-2573-2574-2575-2576-2577-2578-2579-2580-2581-2582-2583-2584-2585-2586-2587-2588-2589-2590-2591-2592-2593-2594-2595-2596-2597-2598-2599-2600-2601-2602-2603-2604-2605-2606-2607-2608-2609-2610-2611-2612-2613-2614-2615-2616-2617-2618-2619-2620-2621-2622-2623-2624-2625-2626-2627-2628-2629-2630-2631-2632-2633-2634-2635-2636-2637-2638-2639-2640-2641-2642-2643-2644-2645-2646-2647-2648-2649-2650-2651-2652-2653-2654-2655-2656-2657-2658-2659-2660-2661-2662-2663-2664-2665-2666-2667-2668-2669-2670-2671-2672-2673-2674-2675-2676-2677-2678-2679-2680-2681-2682-2683-2684-2685-2686-2687-2688-2689-2690-2691-2692-2693-2694-2695-2696-2697-2698-2699-2700-2701-2702-2703-2704-2705-2706-2707-2708-2709-2710-2711-2712-2713-2714-2715-2716-2717-2718-2719-2720-2721-2722-2723-2724-2725-2726-2727-2728-2729-2730-2731-2732-2733-2734-2735-2736-2737-2738-2739-2740-2741-2742-2743-2744-2745-2746-2747-2748-2749-2750-2751-2752-2753-2754-2755-2756-2757-2758-2759-2760-2761-2762-2763-2764-2765-2766-2767-2768-2769-2770-2771-2772-2773-2774-2775-2776-2777-2778-2779-2780-2781-2782-2783-2784-2785-2786-2787-2788-2789-2790-2791-2792-2793-2794-2795-2796-2797-2798-2799-2800-2801-2802-2803-2804-2805-2806-2807-2808-2809-2810-2811-2812-2813-2814-2815-2816-2817-2818-2819-2820-2821-2822-2823-2824-2825

1

1

Destination Tank PO-1, Regenerated Oil for Repair
PO-2, Product for Vendor Transfer

FORM 2

Florida Transformer, Inc
PCB-1000 Operation Log

System Configuration


[Instrument]

Instrument Name : EQL-2
 Instrument Type : GC-17A V3
 Communication Type : RS-232C COM4

Sample Information

Analysis Date & Time : 8/17/2012 7:25:09 AM
 User Name : Admin
 Vial# : 150
 Sample Name : 954322
 Sample ID :
 Sample Type : Unknown
 Injection Volume : 2.00
 Dilution Factor : 10
 Sample Amount : 0.055
 Level# : 1
 Data Name : C:\GCsolution\Data\Project1\954322.gcd
 Method Name : C:\GCsolution\Data\Project1\EQL-2) 8082-073112 eMDL.gcm
 Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
 Batch Name : C:\GCsolution\Data\Project1\EQL-2) TM081412.gcb

Chromatogram 954322 C:\GCsolution\Data\Project1\954322.gcd - Channel 1

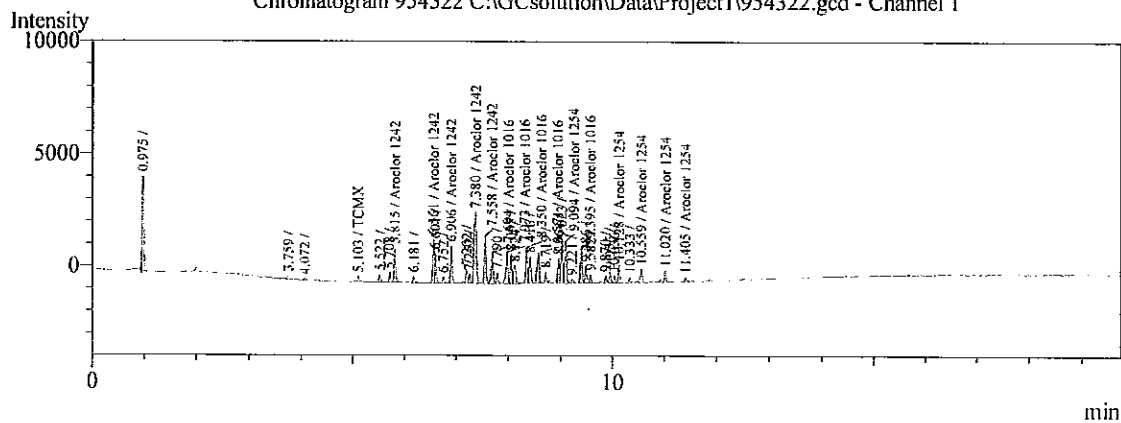

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	51.099	ppm	3383	1526
2	Aroclor 1242	45.208	ppm	4215	1912
3	Aroclor 1242	43.924	ppm	3751	1654
4	Aroclor 1242	50.019	ppm	11353	3159
5	Aroclor 1242	48.632	ppm	4809	2107
6	Aroclor 1016	33.659	ppm	3240	1388
7	Aroclor 1016	30.383	ppm	3453	1392
8	Aroclor 1016	32.021	ppm	3634	1604
9	Aroclor 1016	36.369	ppm	4112	1361
10	Aroclor 1016	39.793	ppm	3913	1556
11	Aroclor 1254	28.461	ppm	4704	1900
12	Aroclor 1254	7.519	ppm	1795	798
13	Aroclor 1254	6.417	ppm	1548	609
14	Aroclor 1254	7.755	ppm	1192	499
15	Aroclor 1254	2.398	ppm	512	198
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.000	ppm	0	0
20	Aroclor 1260	0.000	ppm	0	0
21	TCMX	166.903	%	502	244
Total				56118	21905

1242 47.78
 48

System Configuration


[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

Sample Information

Analysis Date & Time : 9/1/2012 9:17:37 AM
User Name : Admin
Vial# : 1
Sample Name : PO-1K(A)
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 10
Sample Amount : 0.0554
Level# : 1
Data Name : C:\GCsolution\Data\Project1\PO-1K(A).gcd
Method Name : C:\GCsolution\Data\Project1\EQL-3) 8082-081612 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-3 JP090112.gcb

*Post reaction
22 liters Na*

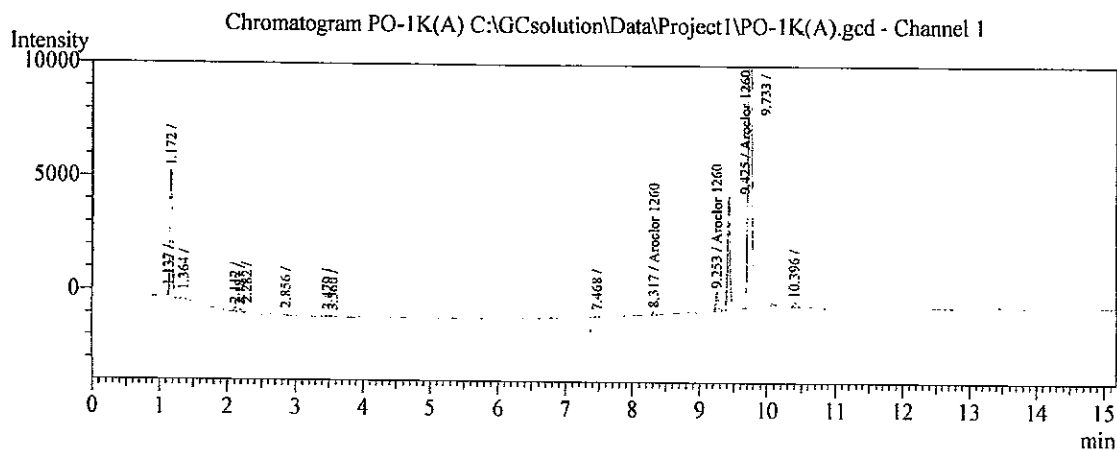

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	0.000	ppm	0	0
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	0.000	ppm	0	0
16	Aroclor 1260	-4.642	ppm	387	155
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	13.699	ppm	2119	853
20	Aroclor 1260	91.794	ppm	12662	5003
21	TCMX	0.000	%	0	0
Total				15168	6011

< 1 ppm

[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

System Configuration

954322

remainders of
954322

MT-4

Analysis Date & Time : 9/3/2012 9:05:03 AM

User Name : Admin

Vial# : 1

Sample Name : PO-2A 090312

Sample ID :

Sample Type : Unknown

Injection Volume : 2.00

Dilution Factor : 10

Sample Amount : 0.0577

Level# : 1

Data Name : C:\GCsolution\Data\Project1\PO-2A 090312.gcd

Method Name : C:\GCsolution\Data\Project1\EQL-3) 8082-081612 eMDL.gcm


Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr

Batch Name : C:\GCsolution\Data\Project1\EQL-3 JP090312.gcb

Sample Information

Intensity

Chromatogram PO-2A 090312 C:\GCsolution\Data\Project1\PO-2A 090312.gcd - Channel 1

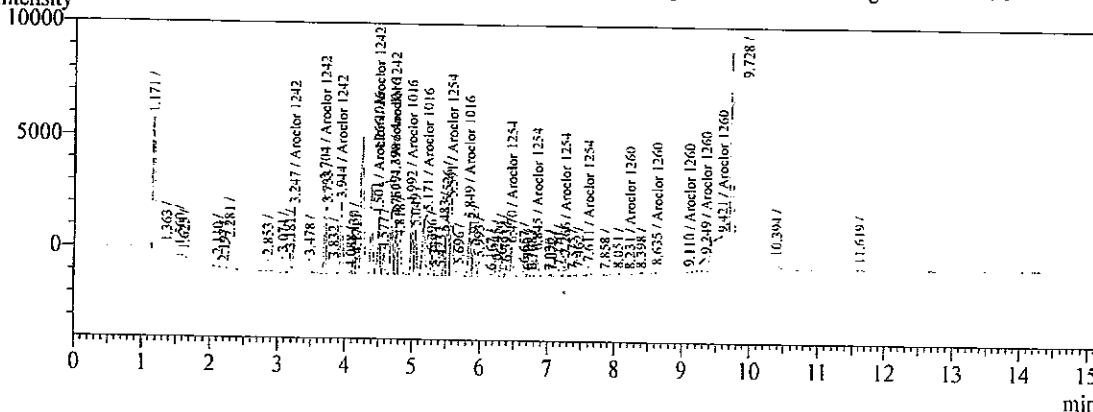

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	43.425	ppm	6100	2884
2	Aroclor 1242	29.493	ppm	7779	4046
3	Aroclor 1242	45.923	ppm	7228	3175
4	Aroclor 1242	44.665	ppm	20291	6139
5	Aroclor 1242	44.050	ppm	8448	3955
6	Aroclor 1016	30.334	ppm	5493	2473
7	Aroclor 1016	32.819	ppm	5904	2843
8	Aroclor 1016	33.387	ppm	6333	3031
9	Aroclor 1016	38.137	ppm	7327	2423
10	Aroclor 1016	33.889	ppm	6073	2398
11	Aroclor 1254	28.354	ppm	8443	3339
12	Aroclor 1254	6.807	ppm	2978	1316
13	Aroclor 1254	5.428	ppm	2431	983
14	Aroclor 1254	6.518	ppm	1739	779
15	Aroclor 1254	2.572	ppm	940	432
16	Aroclor 1260	-5.718	ppm	123	70
17	Aroclor 1260	-2.319	ppm	346	182
18	Aroclor 1260	-3.814	ppm	203	92
19	Aroclor 1260	0.779	ppm	784	348
20	Aroclor 1260	21.749	ppm	3337	1294
21	TCMX	0.000	%	0	0
Total				102301	42202

1242 35.161
36

[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

System Configuration

Analysis Date & Time : 9/3/2012 10:50:57 AM

User Name : Admin

Vial# : 3

Sample Name : PO-2B 090312

Sample ID :

Sample Type : Unknown

Injection Volume : 2.00

Dilution Factor : 10

Sample Amount : 0.0499

Level# : 1


Data Name : C:\GCsolution\Data\Project1\PO-2B 090312.gcd

Method Name : C:\GCsolution\Data\Project1\ (EQL-3) 8082-081612 eMDL.gcm

Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr

Batch Name : C:\GCsolution\Data\Project1\EQL-3 JP090312.gcb

Sample Information

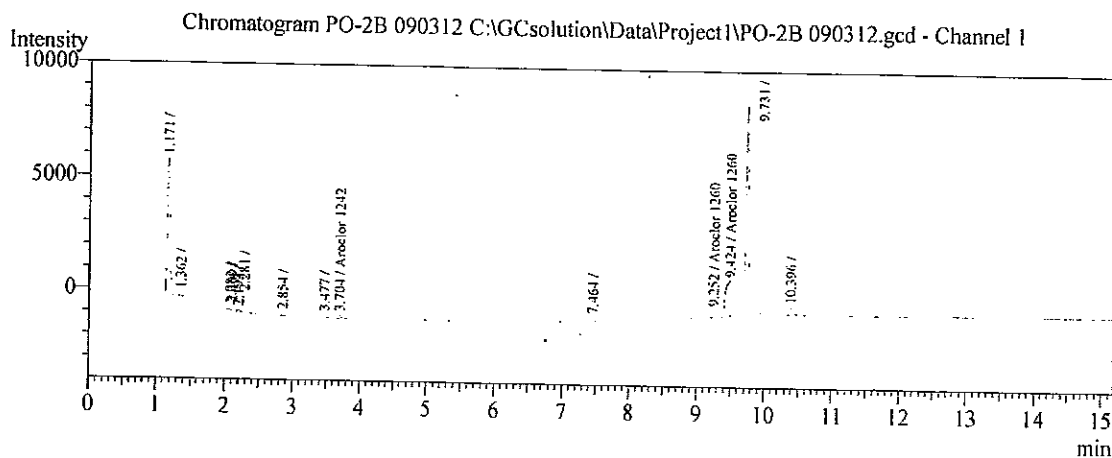

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	1.154	ppm	263	135
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	0.000	ppm	0	0
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.410	ppm	738	327
20	Aroclor 1260	25.794	ppm	3415	1332
21	TCMX	0.000	%	0	0
Total				4417	1794


System Configuration

[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

Sample Information

Analysis Date & Time : 9/3/2012 9:05:03 AM
User Name : Admin
Vial# : 2
Sample Name : PO-3A 090312
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 10
Sample Amount : 0.0548
Level# : 1
Data Name : C:\GCsolution\Data\Project1\PO-3A 090312.gcd
Method Name : C:\GCsolution\Data\Project1\EQL-3 8082-081612 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-3 JP090312.gcb

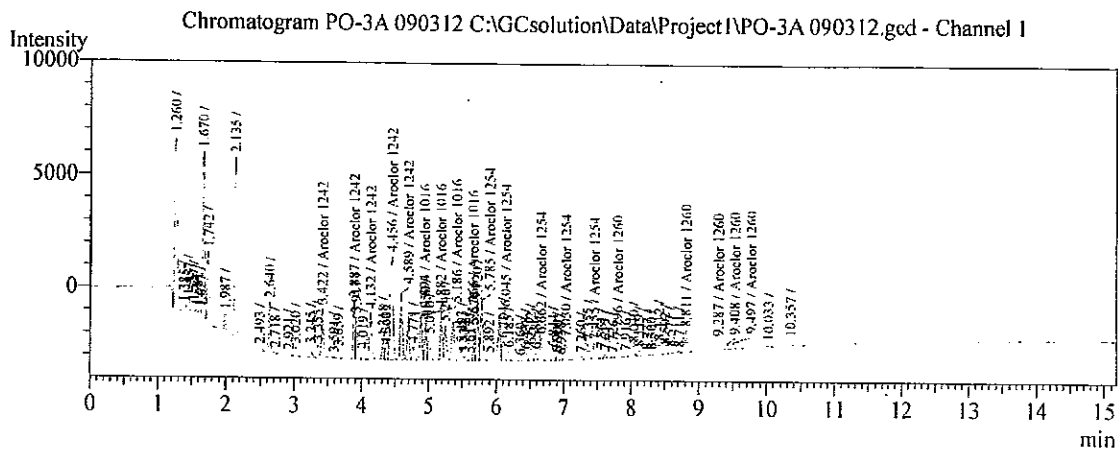

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	24.281	ppm	4589	2190
2	Aroclor 1242	23.755	ppm	5013	2586
3	Aroclor 1242	22.069	ppm	4831	2076
4	Aroclor 1242	23.860	ppm	14791	4610
5	Aroclor 1242	23.500	ppm	6015	2954
6	Aroclor 1016	11.874	ppm	4047	1924
7	Aroclor 1016	11.512	ppm	4044	1952
8	Aroclor 1016	12.080	ppm	4461	2137
9	Aroclor 1016	15.356	ppm	4912	1667
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	9.458	ppm	4874	1956
12	Aroclor 1254	15.648	ppm	6070	2675
13	Aroclor 1254	4.172	ppm	2289	1008
14	Aroclor 1254	4.539	ppm	2640	867
15	Aroclor 1254	4.223	ppm	1496	675
16	Aroclor 1260	-3.848	ppm	1653	691
17	Aroclor 1260	-2.647	ppm	2060	952
18	Aroclor 1260	-3.628	ppm	1029	426
19	Aroclor 1260	-3.730	ppm	429	212
20	Aroclor 1260	-2.352	ppm	530	249
21	TCMX	0.000	%	0	0
Total				75772	31807

1742 2349

23


System Configuration

[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

Sample Information

Analysis Date & Time : 9/4/2012 6:19:39 AM
User Name : Admin
Vial# : 150
Sample Name : PO-3C 090312
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 10
Sample Amount : 0.0533
Level# : 1
Data Name : C:\GCsolution\Data\Project1\PO-3C 090312.gcd
Method Name : C:\GCsolution\Data\Project1\EQL-3 8082-081612 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-3 JP090412.gcb

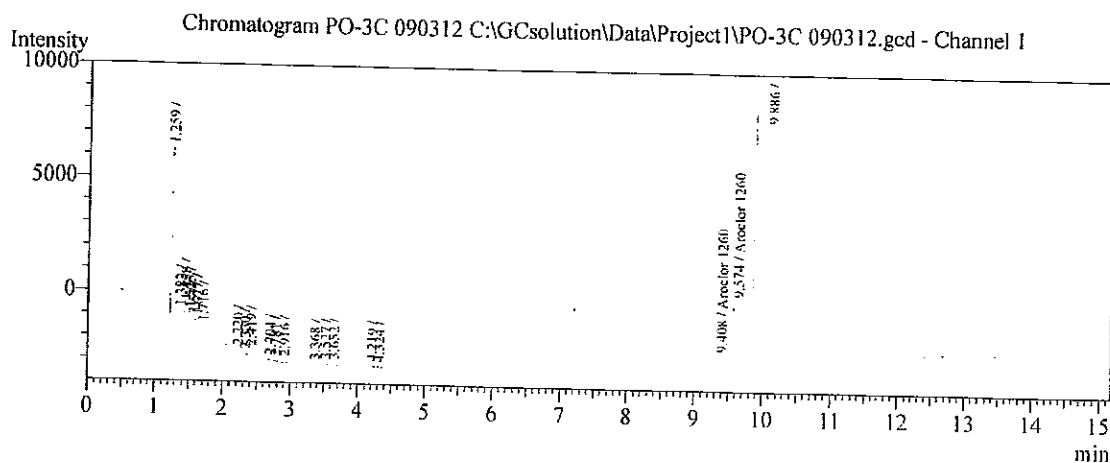

System Configuration


[Instrument]

Instrument Name : EQL-2
 Instrument Type : GC-17A V3
 Communication Type : RS-232C COM4

Sample Information

Analysis Date & Time : 9/4/2012 12:18:43 PM
 User Name : Admin
 Vial# : 150
 Sample Name : PO-4B 090412
 Sample ID :
 Sample Type : Unknown
 Injection Volume : 2.00
 Dilution Factor : 10
 Sample Amount : 0.0543
 Level# : 1
 Data Name : C:\GCsolution\Data\Project1\PO-4B 090412.gcd
 Method Name : C:\GCsolution\Data\Project1\EQL-2) 8082-073112 eMDL.gcm
 Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
 Batch Name : C:\GCsolution\Data\Project1\EQL-2) TM090412.gcb

953050

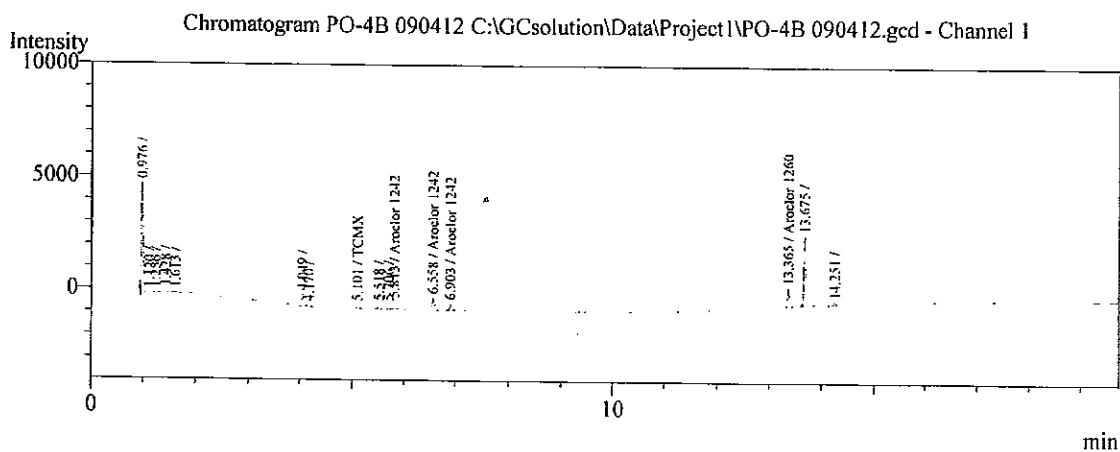

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	10.749	ppm	703	331
2	Aroclor 1242	17.638	ppm	1624	552
3	Aroclor 1242	8.063	ppm	680	281
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	0.000	ppm	0	0
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.000	ppm	0	0
20	Aroclor 1260	19.444	ppm	2098	825
21	TCMX	118.872	%	353	152
Total				5456	2140

1242 12.15
12


System Configuration

[Instrument]
 Instrument Name : EQL-2
 Instrument Type : GC-17A V3
 Communication Type : RS-232C COM4

Sample Information

Analysis Date & Time : 9/4/2012 1:19:15 PM
 User Name : Admin
 Vial# : 150
 Sample Name : PO-4Bx 090412
 Sample ID : 60 min
 Sample Type : Unknown
 Injection Volume : 2.00
 Dilution Factor : 10
 Sample Amount : 0.0517
 Level# : 1
 Data Name : C:\GCsolution\Data\Project1\PO-4Bx 090412 .gcd
 Method Name : C:\GCsolution\Data\Project1\EQ-2) 8082-073112 eMDL.gcm
 Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
 Batch Name : C:\GCsolution\Data\Project1\EQ-2) TM090412.gcb

953050

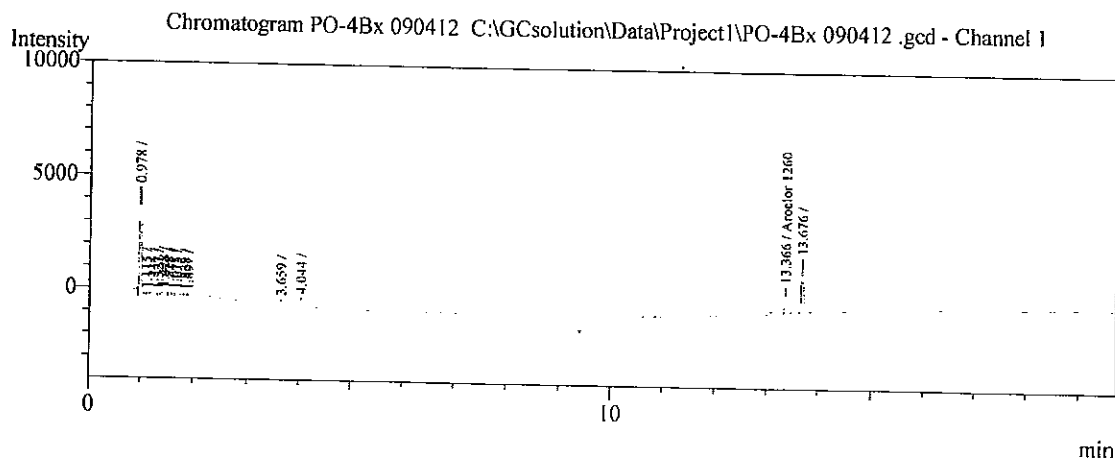

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	0.000	ppm	0	0
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	0.000	ppm	0	0
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.000	ppm	0	0
20	Aroclor 1260	34.072	ppm	3076	1158
21	TCMX	0.000	%	0	0
Total				3076	1158

△

[[Instrument]


Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3

System Configuration

Sample Information

Analysis Date & Time : 9/7/2012 1:51:22 PM
User Name : Admin
Vial# : 150
Sample Name : PO-1A 090713x
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 10
Sample Amount : 0.0499
Level# : 1
Data Name : C:\GCsolution\Data\Project1\PO-1A 090713x.gcd
Method Name : C:\GCsolution\Data\Project1\EQL-3 8082-081612 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-3 TM090412.gcb

Chromatogram PO-1A 090713x C:\GCsolution\Data\Project1\PO-1A 090713x.gcd - Channel 1

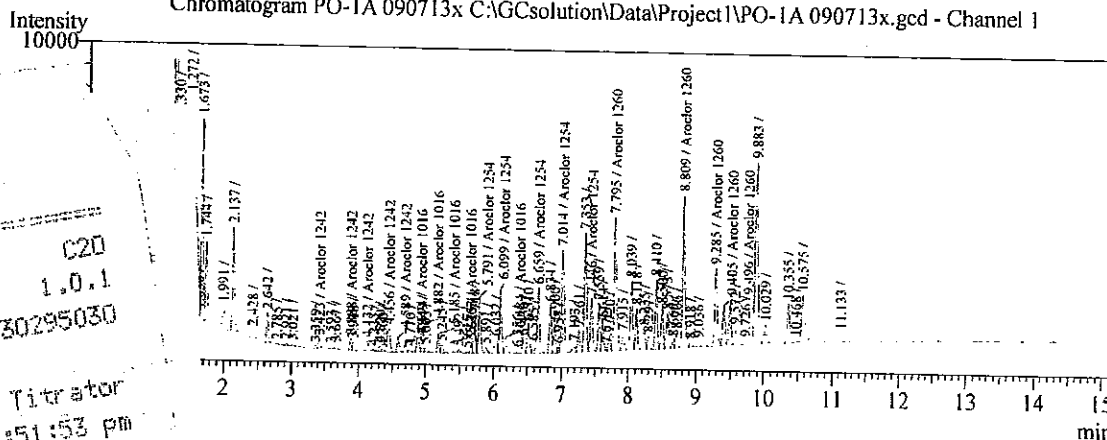

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	4.190	ppm	721	397
2	Aroclor 1242	5.124	ppm	985	526
3	Aroclor 1242	5.870	ppm	1170	441
4	Aroclor 1242	6.015	ppm	3395	1060
5	Aroclor 1242	5.916	ppm	1379	674
6	Aroclor 1016	-4.127	ppm	931	414
7	Aroclor 1016	3.857	ppm	2578	1212
8	Aroclor 1016	-1.037	ppm	1757	836
9	Aroclor 1016	-0.770	ppm	1256	447
10	Aroclor 1016	60.770	ppm	1561	717
11	Aroclor 1254	15.410	ppm	7231	2830
12	Aroclor 1254	17.117	ppm	6046	2548
13	Aroclor 1254	14.844	ppm	7415	2890
14	Aroclor 1254	25.496	ppm	13506	4572
15	Aroclor 1254	18.538	ppm	5978	2386
16	Aroclor 1260	23.741	ppm	15676	5906
17	Aroclor 1260	22.620	ppm	16059	6704
18	Aroclor 1260	23.271	ppm	9244	3437
19	Aroclor 1260	26.775	ppm	4307	1801
20	Aroclor 1260	23.886	ppm	4458	1828
21	TCMX	0.000	%	0	0
				105653	41623

12/11 - 5.1

12/11 - 15.8

12/11 - 24.6
45.5
(46)

LER TOLEDO
ion
al No 5130295030
rator ID
Compact Titrator
07/2012 12:51:53 pm
ministrator

Method ID
Sample series ID

Summary
Samples
No. 1
ID
Sample size 1.6699 g
R1 (Content) 3918.75417 ppm
R2 (Content) 0.3919 %

[Instrument]

Instrument Name : EQL-3
Instrument Type : GC-17A V3
Communication Type : RS-232C COM3


System Configuration

Analysis Date & Time : 9/7/2012 3:46:51 PM
User Name : Admin
Vial# : 150
Sample Name : PO-1B 090712
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 1
Sample Amount : 1
Level# : 1

Sample Information

Data Name : C:\GCsolution\Data\Project1\PO-1B 090712.gcd
Method Name : C:\GCsolution\Data\Project1\EQL-3) 8082-081612 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-3 TM090412.gcb

*SB 10
the significant
impact*

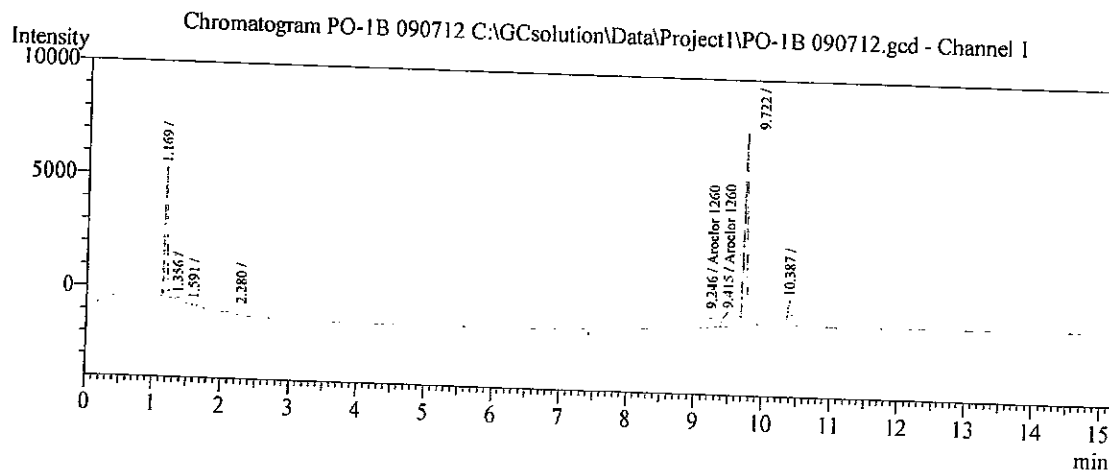

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	0.000	ppm	0	0
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	0.000	ppm	0	0
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.052	ppm	1673	665
20	Aroclor 1260	0.032	ppm	1056	423
21	TCMX	0.000	%	0	0
Total				2728	1087

2


System Configuration

[Instrument]
 Instrument Name : EQL-2
 Instrument Type : GC-17A V3
 Communication Type : RS-232C COM4

Sample Information

Analysis Date & Time : 9/9/2012 3:35:49 PM
 User Name : Admin
 Vial# : 2
 Sample Name : PO 2B 090912x
 Sample ID :
 Sample Type : Unknown
 Injection Volume : 2.00
 Dilution Factor : 10
 Sample Amount : 0.0492
 Level# : 1
 Data Name : C:\GCsolution\Data\Project1\PO 2B 090912x.gcd
 Method Name : C:\GCsolution\Data\Project1\EQL-2) 8082-073112 eMDL.gcm
 Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
 Batch Name : C:\GCsolution\Data\Project1\EQL-2) TM090412jj.gcb

MT-4, post Na (3 litars)
 from 9/9/12

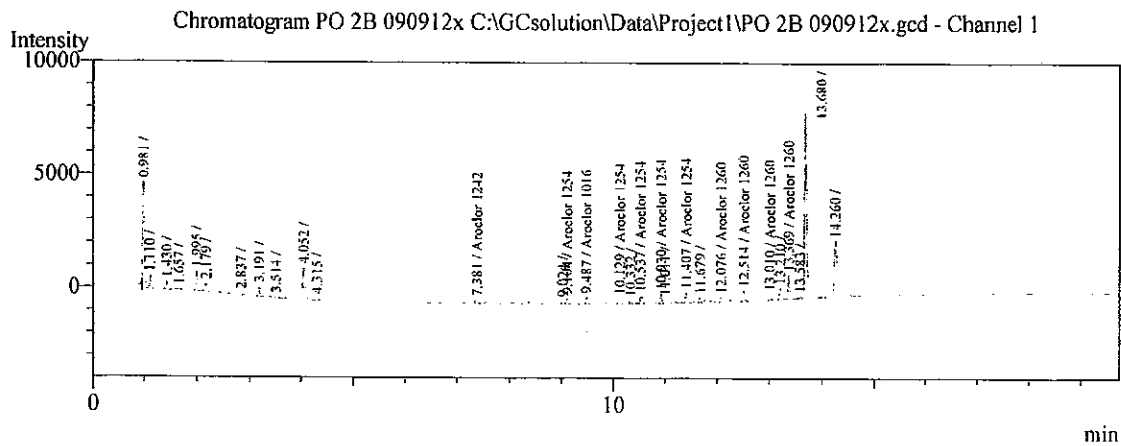

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	0.000	ppm	0	0
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	2.816	ppm	572	169
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	-4.052	ppm	683	316
11	Aroclor 1254	4.160	ppm	615	266
12	Aroclor 1254	3.196	ppm	683	266
13	Aroclor 1254	5.387	ppm	1162	366
14	Aroclor 1254	6.627	ppm	911	434
15	Aroclor 1254	6.058	ppm	1156	462
16	Aroclor 1260	-8.468	ppm	460	215
17	Aroclor 1260	-7.944	ppm	1112	472
18	Aroclor 1260	-6.383	ppm	581	237
19	Aroclor 1260	0.000	ppm	0	0
20	Aroclor 1260	33.136	ppm	2894	1044
21	TCMX	0.000	%	0	0
Total				10830	4246

254
 509

5

System Configuration


[Instrument]

Instrument Name : EQL-2
Instrument Type : GC-17A V3
Communication Type : RS-232C COM4

Sample Information

Analysis Date & Time : 9/10/2012 9:15:15 AM
User Name : Admin
Vial# : 4
Sample Name : PO 2C 091012
Sample ID :
Sample Type : Unknown
Injection Volume : 2.00
Dilution Factor : 10
Sample Amount : 0.0561
Level# : 1
Data Name : C:\GCsolution\Data\Project1\PO 2C 091012.gcd
Method Name : C:\GCsolution\Data\Project1\EQL-2) 8082-073112 eMDL.gcm
Report Name : C:\GCsolution\Data\Project1\PCB RPT 042612 drop.gcr
Batch Name : C:\GCsolution\Data\Project1\EQL-2) TM091012.gcb

MT-4 (3+2liters)
post Na from 9/9/12

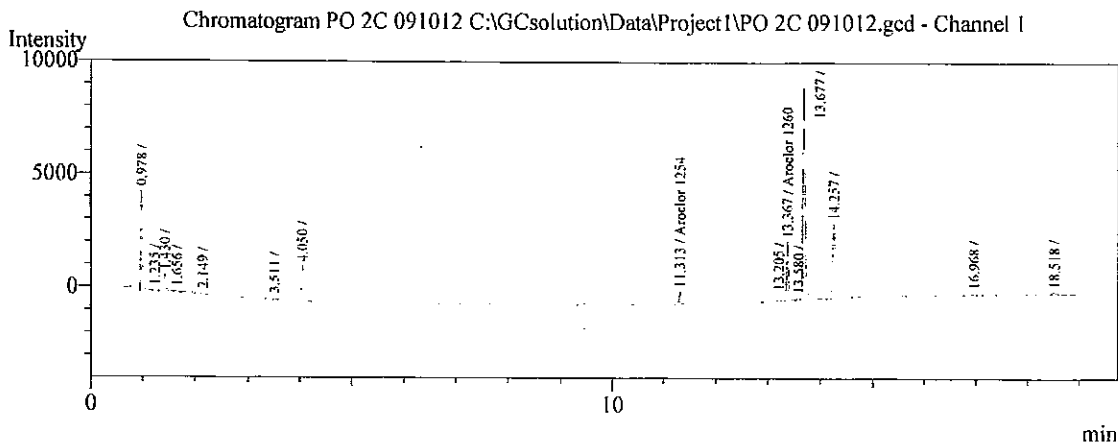

Group Results - Channel 1

Group#	Name	Conc.	Unit	Area	Height
1	Aroclor 1242	0.000	ppm	0	0
2	Aroclor 1242	0.000	ppm	0	0
3	Aroclor 1242	0.000	ppm	0	0
4	Aroclor 1242	0.000	ppm	0	0
5	Aroclor 1242	0.000	ppm	0	0
6	Aroclor 1016	0.000	ppm	0	0
7	Aroclor 1016	0.000	ppm	0	0
8	Aroclor 1016	0.000	ppm	0	0
9	Aroclor 1016	0.000	ppm	0	0
10	Aroclor 1016	0.000	ppm	0	0
11	Aroclor 1254	0.000	ppm	0	0
12	Aroclor 1254	0.000	ppm	0	0
13	Aroclor 1254	0.000	ppm	0	0
14	Aroclor 1254	0.000	ppm	0	0
15	Aroclor 1254	6.082	ppm	1324	560
16	Aroclor 1260	0.000	ppm	0	0
17	Aroclor 1260	0.000	ppm	0	0
18	Aroclor 1260	0.000	ppm	0	0
19	Aroclor 1260	0.000	ppm	0	0
20	Aroclor 1260	84.698	ppm	7220	2578
21	TCMX	0.000	%	0	0
Total				8544	3137

4